




Optical Coherence Tomography

Retina Scan Duo™

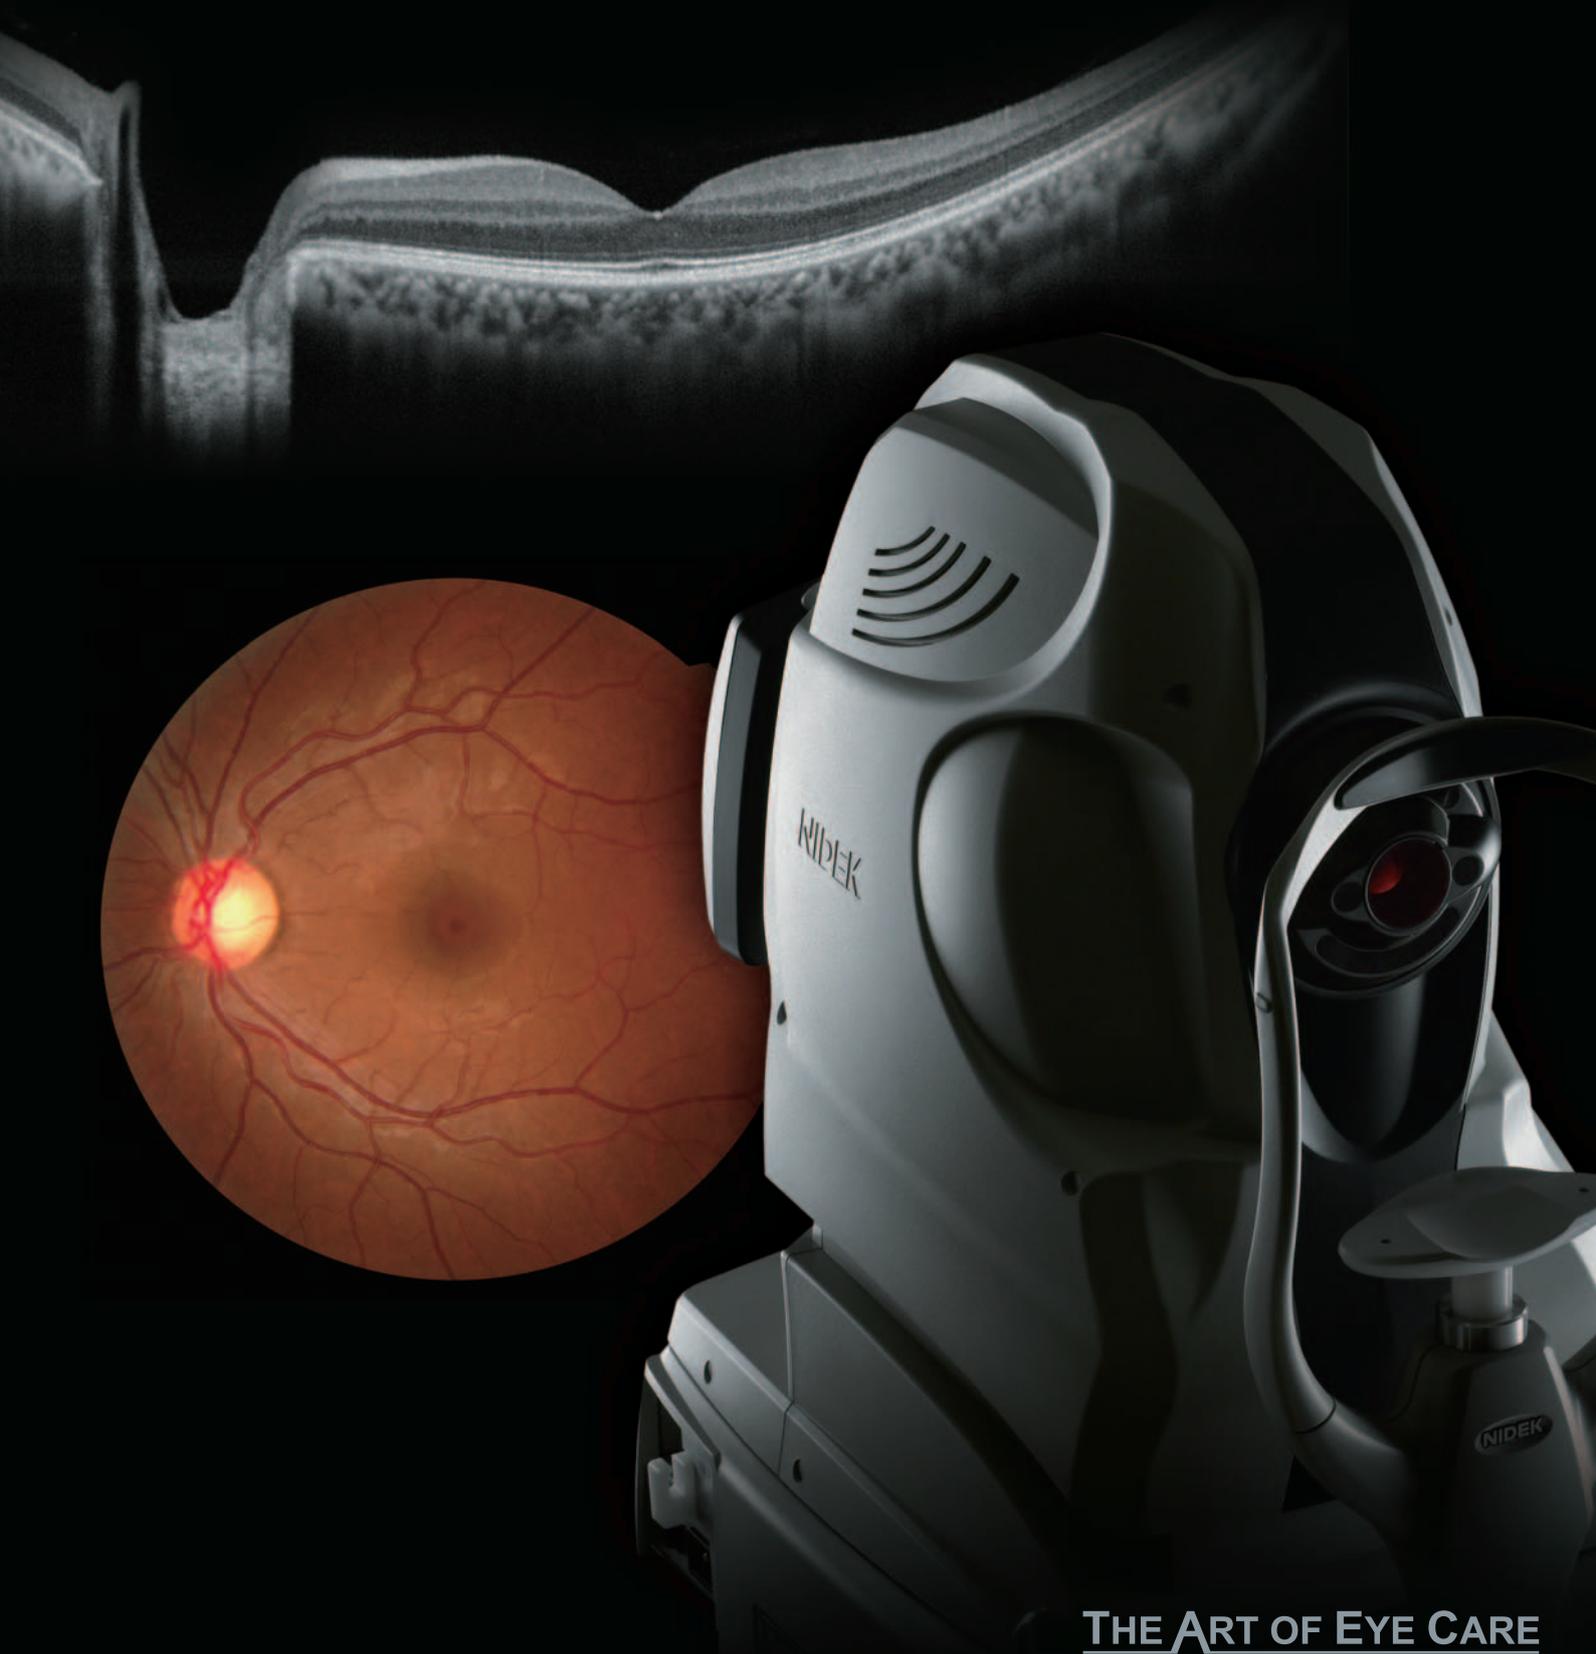

THE ART OF EYE CARE



*High Definition OCT & Fundus Imaging
in One Compact System*



A
a pl
Pursuit
fo



Retina Scan Duo

The *Retina Scan Duo*™ is a combined OCT and fundus camera system that is a user friendly and versatile unit providing high definition images and value added features.

The intuitive software, the automated functions, the rapid measurements and high-quality images make the *Retina Scan Duo*™ a pleasure to operate, akin to photography that captures many of the vivid landscapes experienced over your lifetime. The combination of features results in a better overall experience for the patient and practitioner.

Additional value added features include fundus autofluorescence and En face OCT.

device that is
easy to use
stunning clarity
for everyone




High Quality
&
Versatility



User Friendly



Value Added
Features

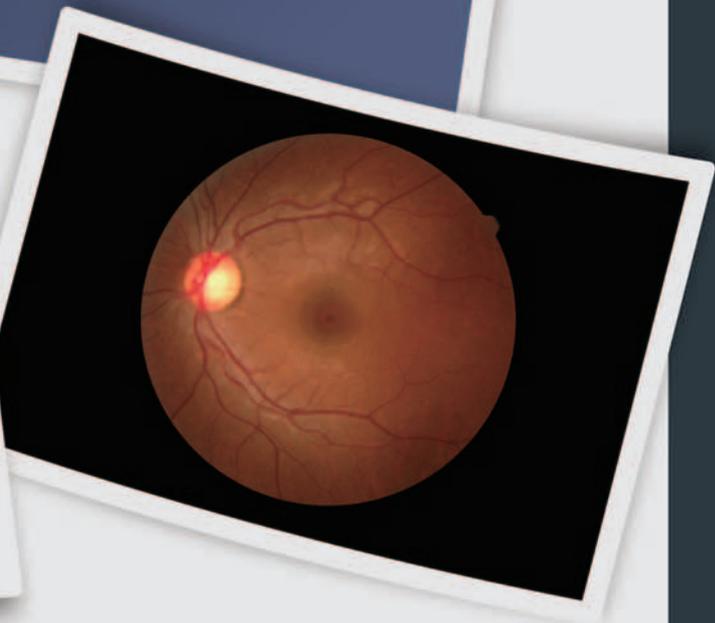



User Friendly

NIDEK 3-D auto tracking, auto shot, and a user friendly interface allow rapid and easy image capturing. Combining an OCT and fundus camera in one system saves time and space, and improves the diagnostic workflow and efficiency.


● User Friendly Interfaces for Two Capture Modes

Standard and professional modes are available.

Each mode has a different image capture interface which can be selected based on clinic preference.

Standard Mode


for general screening and analysis

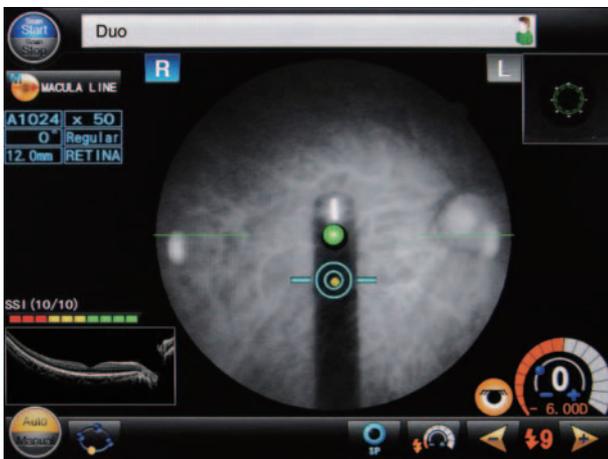

In the standard mode, operation is as simple as a fundus camera, which is helpful for daily practice.

Professional Mode

for advanced screening and analysis

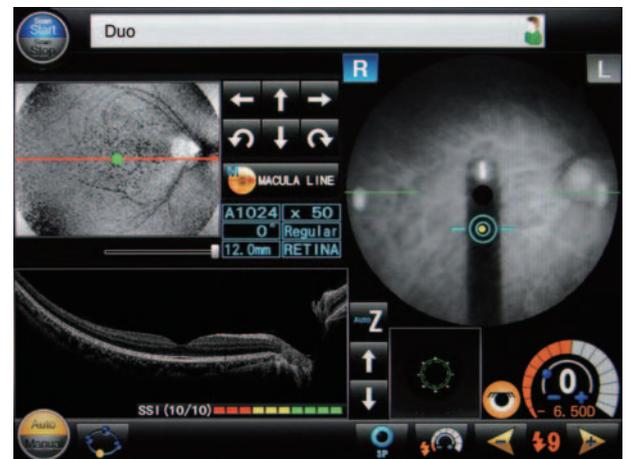

The professional mode is favored for advanced, detailed screening and analysis. In this mode, the scanning position can be adjusted to the phase fundus image and it supports capturing precise OCT images.

Easy

User Friendly



● 3-D Auto Tracking and Auto Shot


The acclaimed 3-D auto tracking and auto shot functions allow easy imaging of the fundus and all its features. Once alignment is completed, both the OCT and fundus images can be captured in a single shot.

● Operation with Joystick for Flexible Alignment

The joystick helps the operator make fine adjustments during alignment to improve the precision, even for eyes with poor fixation which cannot be tracked with automated tracking systems.

● Space-saving Unit

The small footprint replaces two units with one combined unit.

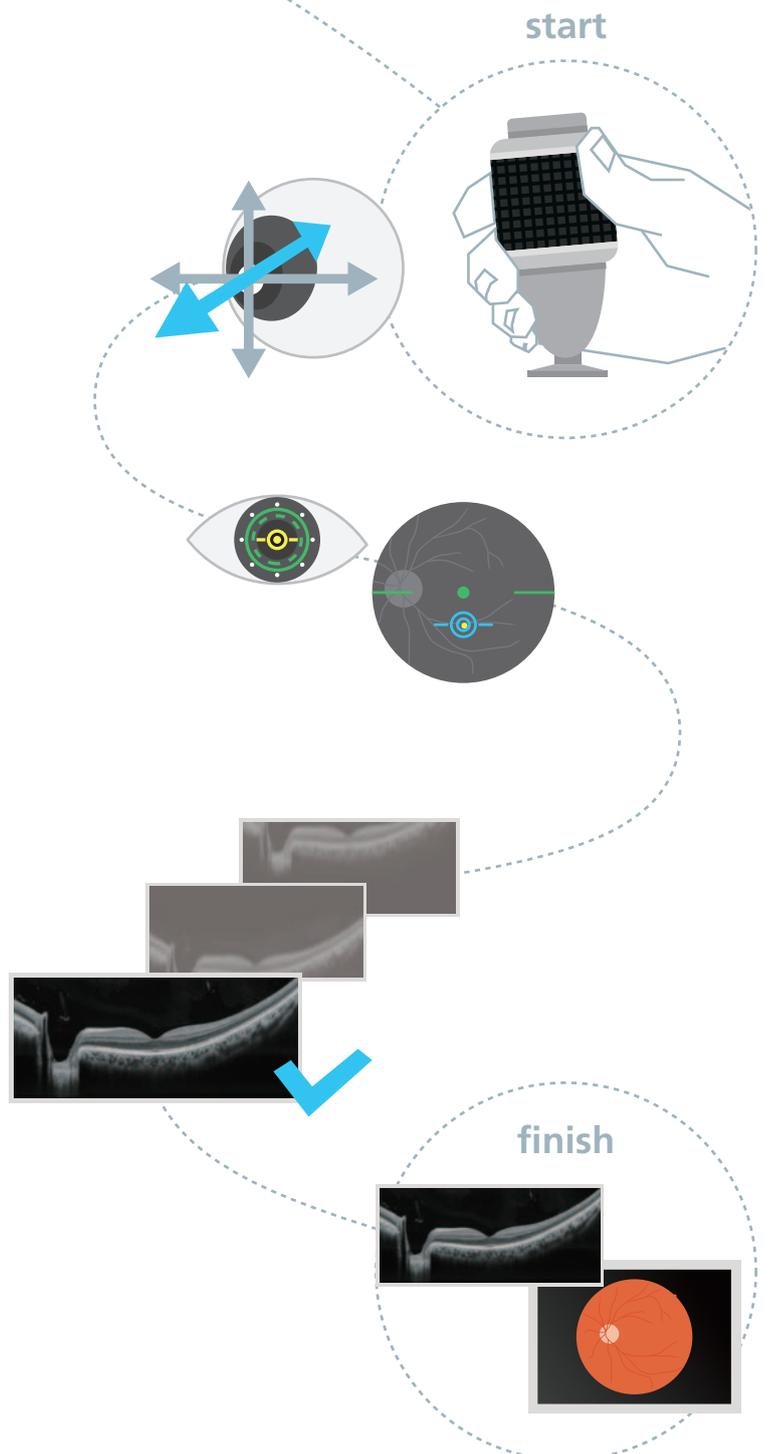


★★★ High Quality & Versatility

The OCT and fundus imaging are high definition images that are comparable in quality to the standard NIDEK OCT system and fundus camera. The Retina Scan Duo™ is versatile enough to be tailored to the individual diagnostic requirements for any practitioner.

OCT


- HD Image Averaging (max. 50 images)
- Selectable OCT Sensitivity – ultra fine, fine, regular

Selecting the OCT sensitivity based on ocular pathology allows image capture with higher definition or at high speed. Ultra fine and fine sensitivities are used to capture high definition images and regular sensitivity is used to capture images at high speed.

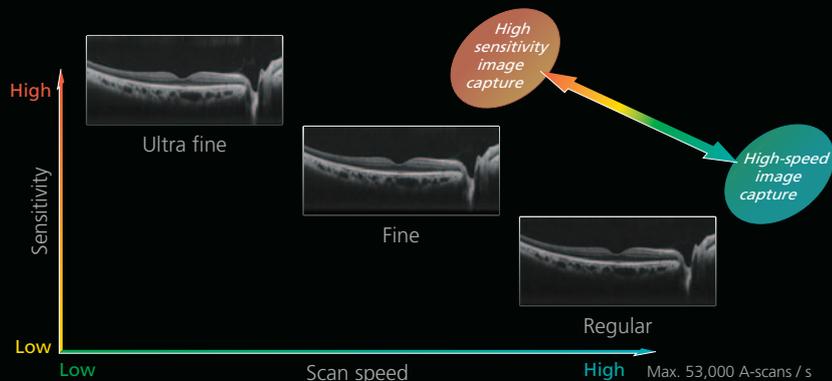

● Enhanced Image

The image enhancement function allows adjustment to image brightness for advanced image quality and details.

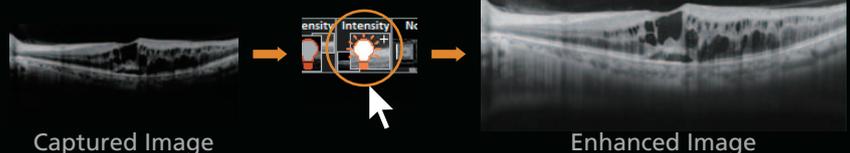

● Wide Area Scan (12 x 9 mm) / Wide Area Normative Database

A 12 x 9 mm wide area image centered on the macula can be captured with the Retina Scan Duo™. The 9 x 9 mm normative database provides a color-coded map indicating distribution range of the patient's macular thickness in a population of normal eyes.

● Multiple OCT Scan Patterns

A wide range of scanning patterns is available to allow the practitioner to select a scan that suits the retinal region and ocular pathology.

* The anterior segment adapter is optional.



Fundus Camera

● 12-megapixel CCD Camera

The Retina Scan Duo™ has a built-in 12-megapixel CCD camera, producing high quality fundus images.

● Stereo and Panorama Photography


The Retina Scan Duo™ navigates stereo and panorama photography with target marks displayed on an observation screen, which enables an operator to easily capture stereo images and a panorama composition.

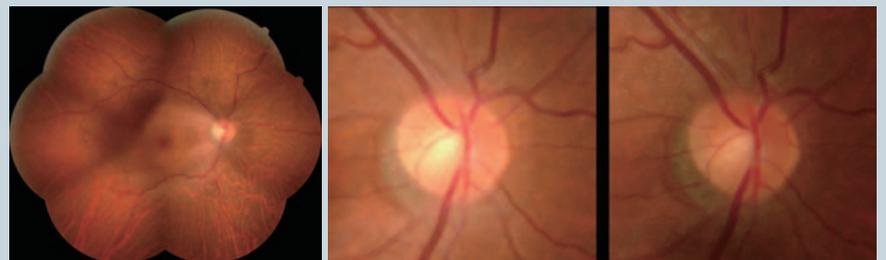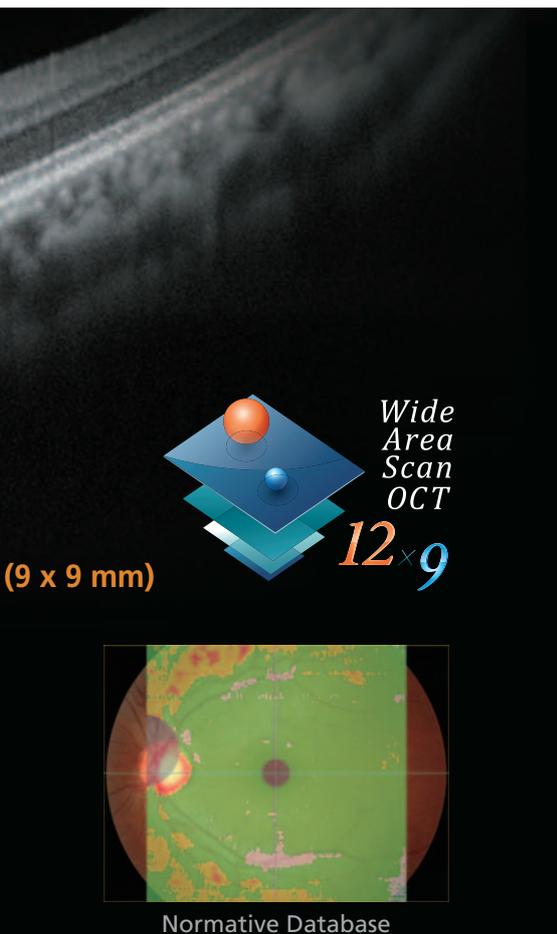

Panorama

Stereo Images

» Retina: 8 patterns

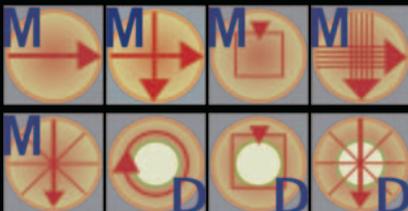

» Anterior*: 4 patterns






Value Added Features

In addition to combining standard OCT and fundus camera features, the Retina Scan Duo™ offers additional diagnostic features allowing the practitioner to stay a step ahead of current standards.

● Fundus Autofluorescence (FAF)*1

The fundus autofluorescence (FAF) function is an advanced screening feature. The FAF is a non-invasive method to evaluate the RPE without contrast dye. The function is helpful for detecting early stage retinal disorders.

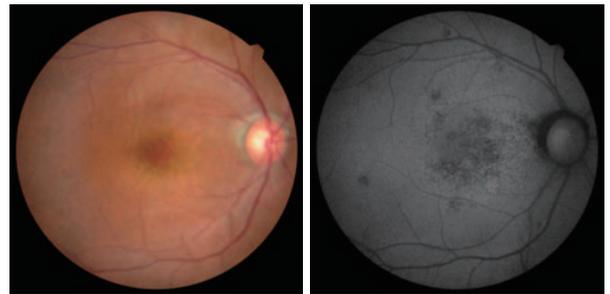


Color Fundus Image*2

FAF Image*2

● En face OCT

En face OCT imaging is for advanced studies of retinal pathology including factors that compromise photoreceptor function and retinal and choroidal vasculature.

- A. Thickness Map (ILM - RPE / BM)
- B. En face (IPL / INL Offset: +121 μm, Thickness: 42 μm)
- C. B-scan Image
- 1. En face (ILM Offset: 0 μm, Thickness: 42 μm)
- 2. En face (IPL / INL Offset: +21 μm, Thickness: 42 μm)
- 3. En face (RPE / BM Offset: -41 μm, Thickness: 42 μm)
- 4. En face (RPE / BM Offset: 0μm, Thickness: 125 μm)

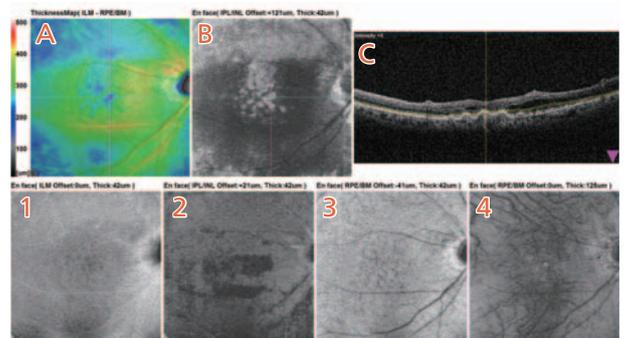

En face OCT Image

● NAVIS-EX

NAVIS-EX is an image filing software, which networks the Retina Scan Duo™ and other NIDEK diagnostic devices. This functionality enhances the capability of the diagnostic device with additional features and increases clinical efficiency.

- Analysis and report
- Normative database
- Long axial length normative database*3
- DICOM connectivity



Optical Shop



Hospital



Clinic






● Anterior Segment Adapter*4

The anterior segment adapter enables observation and analyses of the anterior segment.



Angle Measurement


- ACA
Angle between posterior corneal surface and iris surface
- AOD500 (AOD750)
Distance between iris and a point 500 μm (or 750 μm) from the scleral spur on posterior corneal surface
- TISA500 (TISA750)
Area circumscribed with AOD500 (or AOD750) line, posterior corneal surface, line drawn from scleral spur in parallel with AOD line, and the iris surface

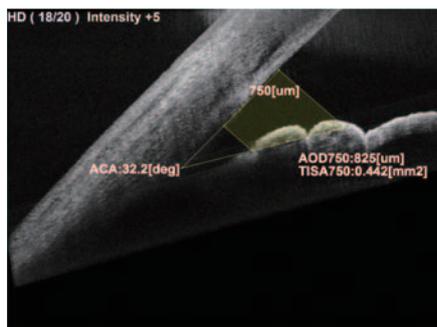


Angle Measurement

Corneal Measurement

- Corneal thickness
Corneal thickness of apex and user selected sites
- Corneal thickness map
Map of corneal thickness plotted radially



Thickness Map

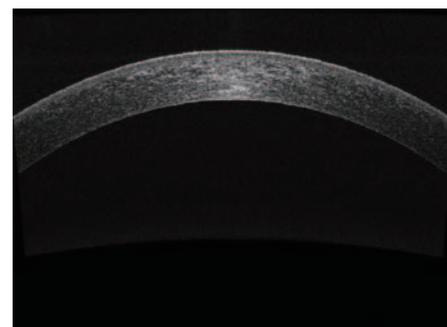


Corneal Measurement


*1 The fundus autofluorescence (FAF) function is available for the FAF model. *2 Photos courtesy of Kariya Toyota General Hospital. *3 The long axial length normative database is an optional software. *4 The anterior segment adapter is optional.

Glaucoma


Macula Map (both eyes)

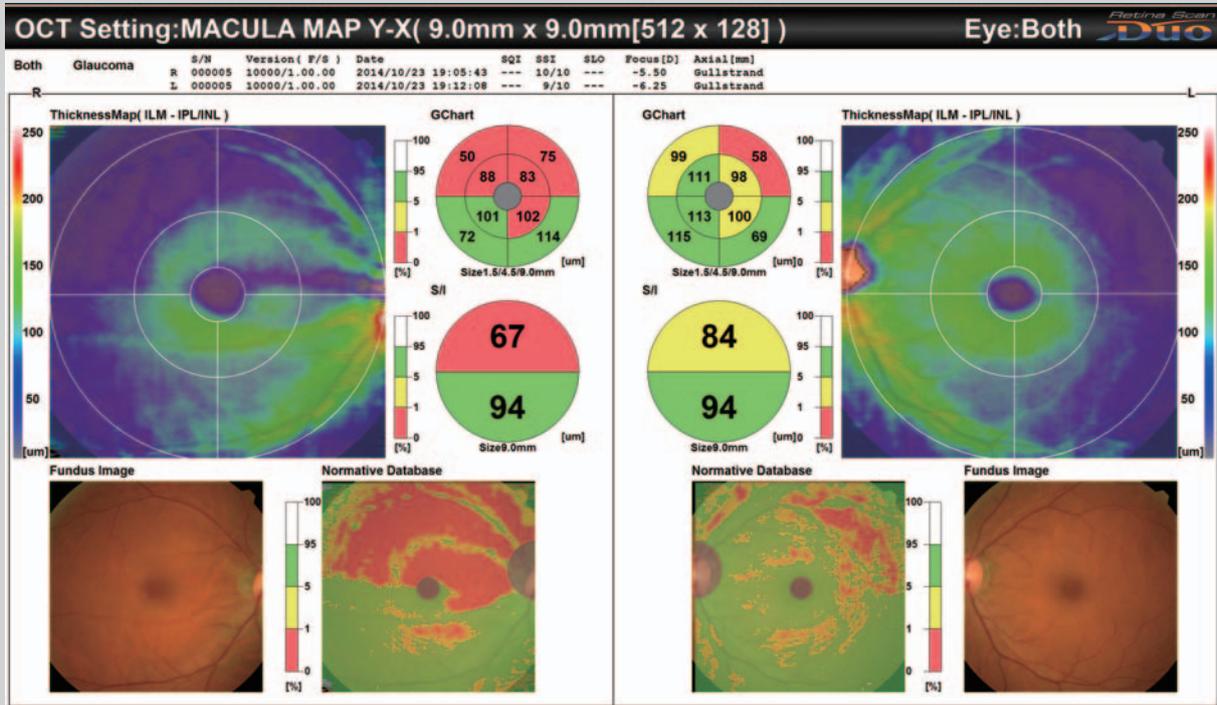


Disc Map (both eyes)

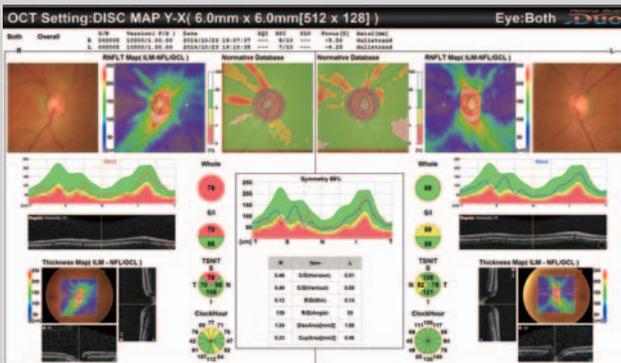

Customized Report

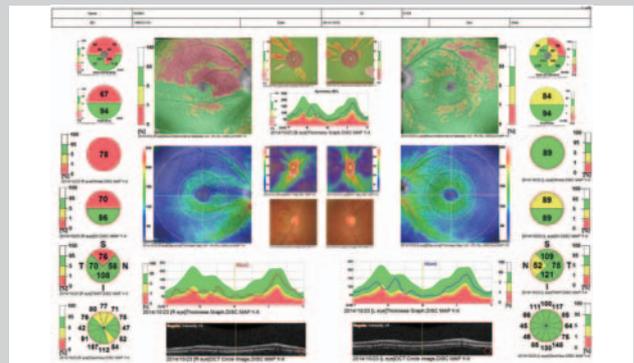


Glaucoma Follow-up

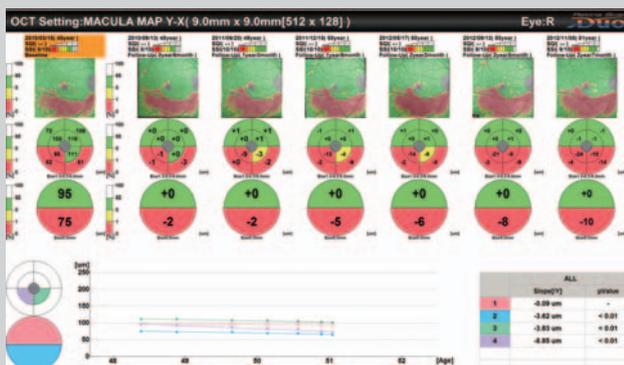


Anterior Chamber Angle Line Scan*

Macula


Macula Line (both eyes)

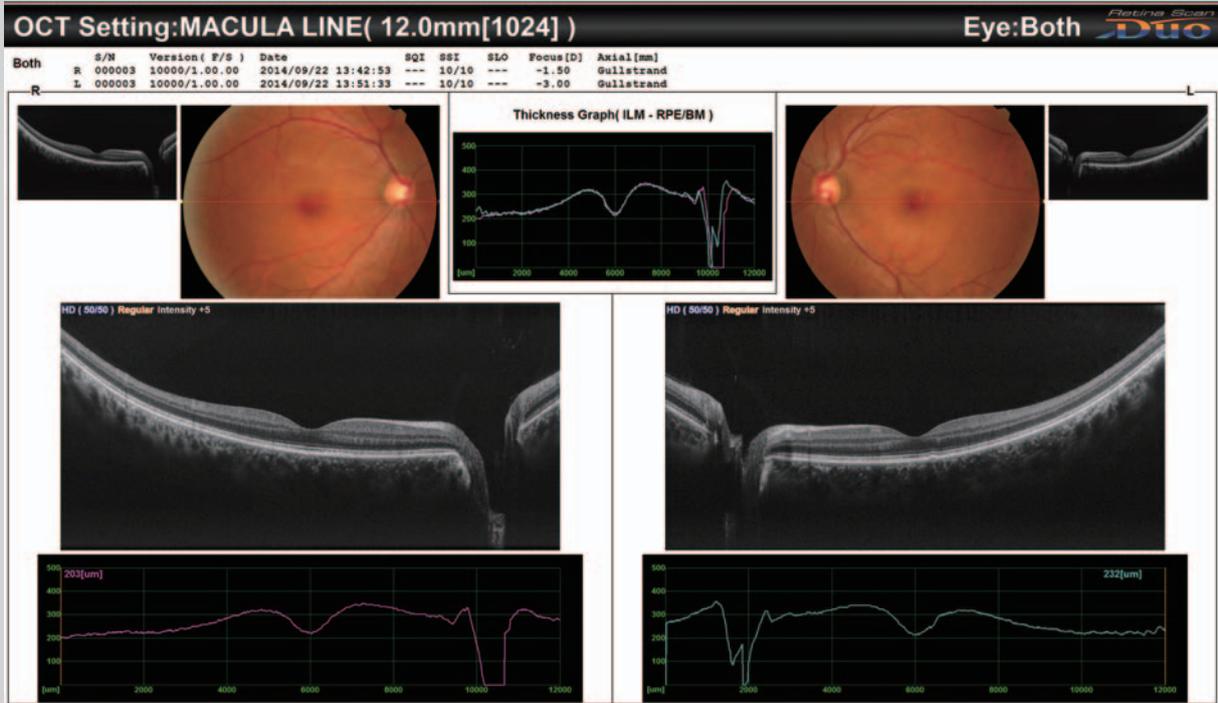


3-D Macula Map (one eye)

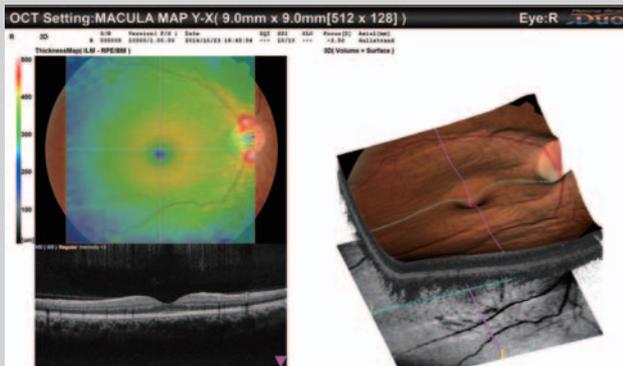


En face

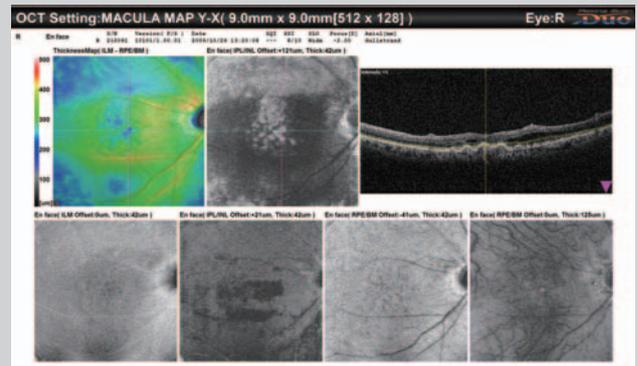

Macula Radial (both eyes)

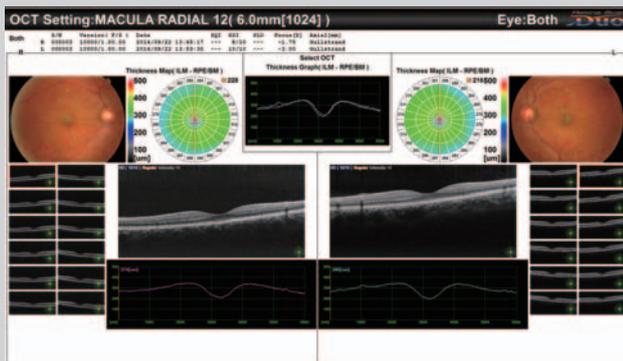

Macula Map (one eye)

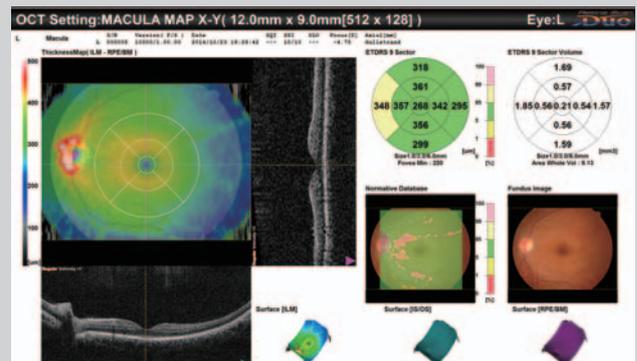

Retina Scan Duo™ RS-330 Specifications

OCT	
OCT scanning	
Principle	Spectral domain OCT
Optical resolution	Z: 7 µm, X-Y: 20 µm
Scan range	X: 3 to 12 mm Y: 3 to 9 mm Z: 2.1 mm
Digital resolution	Z: 4 µm, X-Y: 3 µm
OCT light source	880 nm
Scan speed	Max. 53,000 A-scan / s (regular mode)
Acquisition time of 3-D image	1.6 s (regular mode)
Auto alignment	Z direction
Minimum pupil diameter	ø2.5 mm
Scan patterns	Macula line, macula cross, macula map, macula multi, macula radial, disc circle, disc map, disc radial
Fundus surface imaging	
Principle	OCT phase fundus
Angle of view	40° x 30°
Fundus camera	
Type	Non-mydratiac fundus camera, color, FAF*
Angle of view	45° (33° for small pupil image capture)
Minimum pupil diameter	ø4 mm (ø3.3 mm for small pupil image capture)
Light source	Xenon flash lamp 300 Ws
Flash intensity	17 levels from FL1 (F4.0 +0.8 EV) to FL17 (F16 +0.8 EV) 0.25 EV increments
Camera	Built-in 12-megapixel CCD camera
Common specification	
Working distance	45.7 mm
Display	Tilttable 8.4-inch color LCD
Dioptic compensation for patient's eyes	-33 to +35 D total -33 to -7 D with minus compensation lens -12 to +15 D with no compensation lens +11 to +35 D with plus compensation lens
Internal fixation lamp	LED
Horizontal movement	36 mm (back / forth) 85 mm (right / left)
Vertical movement	32 mm
Chinrest movement	62 mm (up / down, motorized)
Auto tracking	X-Y-Z directions
Auto shot	Available
PC networking	Available
Power supply	AC 100 to 240 V 50 / 60 Hz
Power consumption	350 VA
Dimensions / Mass	370 (W) x 536 (D) x 602 (H) mm / 38 kg (standard model) 39 kg (FAF model) 14.6 (W) x 21.1 (D) x 23.7 (H)" / 84 lbs. (standard model) 86 lbs. (FAF model)
Optional accessories	Anterior segment adapter, external fixation lamp, isolation transformer, motorized optical table, PC rack, long axial length normative database, USB 3.0 PCIE add in card

* The fundus autofluorescence (FAF) function is available for the FAF model.

Product / Model name: Optical Coherence Tomography RS-330
Brochure and listed features of the device are intended for non-US practitioners.
Specifications may vary depending on circumstances in each country.
Specifications and design are subject to change without notice.



HEAD OFFICE
(International Div.)
34-14 Maehama, Hiroishi
Gamagori, Aichi 443-0038,
JAPAN
TEL: +81-533-67-8895
URL: <http://www.nidek.com>
[Manufacturer]

TOKYO OFFICE
(International Div.)
3F Sumitomo Fudosan Hongo
Bldg, 3-22-5 Hongo, Bunkyo-ku,
Tokyo 113-0033, JAPAN
TEL: +81-3-5844-2641
URL: <http://www.nidek.com>

NIDEK INC.
47651 Westinghouse Drive,
Fremont, CA 94539, U.S.A.
TEL: +1-510-226-5700
+1-800-223-9044
(US only)
URL: <http://usa.nidek.com>

NIDEK S.A.
Europarc,
13 rue Auguste Perret,
94042 Créteil, FRANCE
TEL: +33-1-49 80 97 97
URL: <http://www.nidek.fr>

NIDEK TECHNOLOGIES S.R.L.
Via dell'Artigianato,
6/A, 35020 Albignasego (Padova),
ITALY
TEL: +39 049 8629200/8626399
URL: <http://www.nidektechnologies.it>

NIDEK (SHANGHAI) CO., LTD.
Rm3205, Shanghai Multi
Media Park, No.1027 Chang
Ning Rd, Chang Ning District,
Shanghai, CHINA 200050,
TEL: +86 021-5212-7942
URL: <http://www.nidek-china.cn>

NIDEK SINGAPORE PTE. LTD.
51 Changi Business Park
Central 2, #06-14, The
Signature 486066,
SINGAPORE
TEL: +65 6588 0389

Anterior segment adapter (optional)

Scan patterns	Cornea line, cornea cross, cornea radial, ACA line
Software analysis	Corneal thickness measurement, corneal thickness map, angle measurement

Motorized optical table (optional)

Dimensions / Mass	639 (W) x 472 (D) x 599 to 843 (H) mm / 28 kg 25.2 (W) x 18.6 (D) x 23.6 to 33.2 (H)" / 62 lbs.
Power supply	AC 100 V / 220 to 240 V 50 / 60 Hz
Power consumption	200 V type 160 W 100 V type 150 W

PC rack (optional)

Dimensions / Mass	620 (W) x 450 (D) x 700 (H) mm / 29 kg 24.4 (W) x 17.7 (D) x 27.6 (H)" / 64 lbs.
-------------------	---

Isolation transformer (optional)

Dimensions / Mass	130 (W) x 220 (D) x 130 (H) mm / 9 kg 5.1 (W) x 8.7 (D) x 5.1 (H)" / 20 lbs.
Power supply	200 V type Input AC 220 / 230 / 240 V Output AC 220 / 230 / 240 V 50 / 60 Hz 100 V type Input AC 100 / 110 / 120 V Output AC 100 / 110 / 120 V 50 / 60 Hz
Maximum power output	500 VA

